
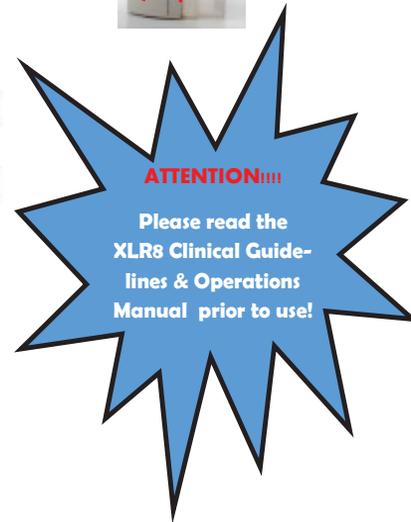


# XLR8 QUICK GUIDE

If you need further assistance, please call your local Custom Medical Solutions Representative, our 24 hour hotline at 1-866-350-5640 or log onto [www.custommedicalsolutions.com](http://www.custommedicalsolutions.com)

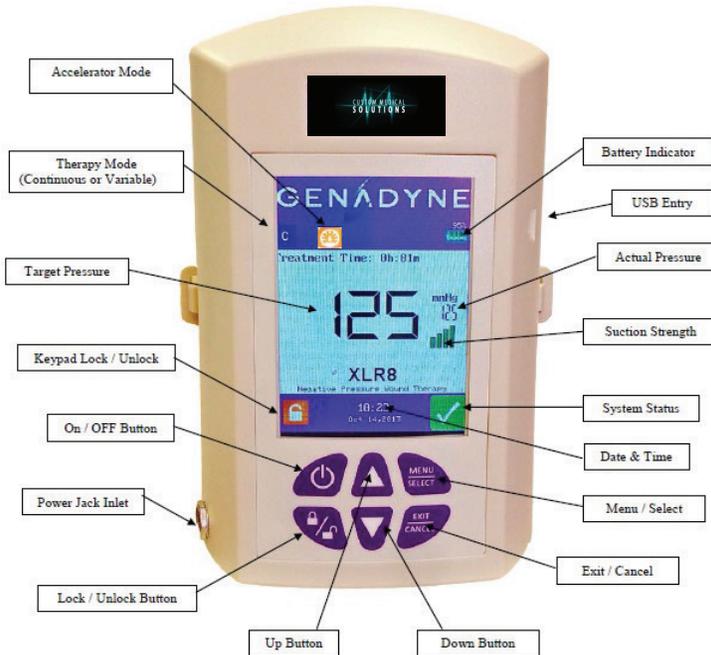

ICONS/ALERTS	✓ ACTION/RESOLUTION	* USER TIPS
--------------	---------------------	-------------

	<p><b>LEAK</b> Indication of a leak in the dressing or canister</p>	<ul style="list-style-type: none"> <li>✓ Check canister/dressing lure lock connector</li> <li>✓ Ensure canister is fully engaged</li> <li>✓ Identify air leaks in the dressing</li> </ul>	<ul style="list-style-type: none"> <li>* Identify air leaks by listening with stethoscope</li> <li>* Use additional drape to patch small air leaks</li> <li>*Make sure dressing is fully collapsed</li> </ul>
	<p><b>BLOCKAGE</b> A blockage is detected between the wound dressing and the canister</p>	<ul style="list-style-type: none"> <li>✓ Check tubing for closed clamps, kinks, crimps, or blockages</li> <li>✓ Inspect to ensure a quarter size (2.5cm) hole has been cut in the drape</li> </ul>	<ul style="list-style-type: none"> <li>*Ensure port pad is on a flat area of the body, avoiding skin folds and creases</li> <li>*Too small of a hole or slit may cause the the dressing to close on itself, pressure fluctuations, and/or other functionality issues</li> </ul>
	<p><b>CANISTER FULL</b> The canister is filled with exudates</p>	<ul style="list-style-type: none"> <li>✓ Change canister and restart therapy</li> <li>✓ If minimal exudate is noted, the Canister filter may have gotten wet. Replace canister and reset the system.</li> </ul>	<ul style="list-style-type: none"> <li>*If canister is not changed immediately, the system will shut down.</li> <li>*Keep the unit upright at all times for optimal performance and to avoid damage to the unit</li> </ul>
	<p><b>LOW BATTERY</b> Battery has less than 2% (&lt;30 min's) operating time left</p>	<ul style="list-style-type: none"> <li>✓ Plug in the XLR8 power adapter to a wall outlet to recharge.</li> <li>✓ Ensure the power cord is securely placed In the XLR8 charge port</li> </ul>	<ul style="list-style-type: none"> <li>*It may take up to 3 hours to fully recharge</li> <li>*Lightning bolt icon indicates recharging</li> <li>*Keep unit plugged in except when transporting or ambulating (*Battery power aprox 12Hrs)</li> </ul>
	<p><b>ACCELERATOR MODE</b> Auto feature will run every *10 min for *15 sec</p>	<ul style="list-style-type: none"> <li>✓ This preset feature will clear exudates from the tubing to ensure that consistent negative pressure is delivered to the wound site.</li> </ul>	<ul style="list-style-type: none"> <li>*During the activation phase, the prescribed therapy numbers may fluctuate a few mm/hg while clearing the line</li> </ul>

- Times are approximate depending on software version being used